

INVESTIGATION OF POSITIONING OF FLUID MUSCLE ACTUATOR UNDER VARIABLE TEMPERATURE

■ ABSTRACT:

Some researchers have mentioned that temperature creates an important part in the accuracy of positioning of pneumatic artificial muscles (PAMs). However, in literature investigations for measuring temperature inside and outside the PAMs have not been found. This paper presents our robust motion control of these muscle actuators under different temperatures using sliding-mode control.

The layout of this paper is as follows. Section 2 (The study) is devoted to display our test-bed and the LabVIEW programs. Section 3 (Results and discussion) presents several experimental results. Finally, section 4 (Conclusions) gives the investigations we plan.

Fluid Muscles DMSP-10-250N-RM-RM (with inner diameter of 10 mm and initial length of 250 mm) produced by Festo company were selected for our newest study.

■ KEYWORDS:

muscle actuators, variable temperature

INTRODUCTION

The working principle of the pneumatic artificial muscles is well described in literature ([1], [2], [3], [4], [5] and [6]).

There are a lot of advantages of these muscles like the high strength, good power-weight ratio, low price, little maintenance needed, great compliance, compactness, inherent safety and usage in rough environments. However, problems with the control of the highly nonlinear pneumatic systems have prevented their widespread use [7]. For this, a fast and robust control necessary to achieve the desired motion. Several control ways have been applied to control different humanoid or robot arms, manipulators, prosthetic and therapy devices driven by pneumatic artificial muscles. The early control methods were based on classical linear controllers and then some modern control strategies have been developed (e. g. adaptive controller, sliding-mode controller, fuzzy controller, neural network controller and others) [8].

The layout of this paper is as follows. Section 2 (The study) is devoted to display our test-bed and the LabVIEW programs. Section 3 (Results and discussion) presents several experimental results. Finally, section 4 (Conclusions) gives the investigations we plan.

Fluid Muscles DMSP-10-250N-RM-RM (with inner diameter of 10 mm and initial length of 250 mm) produced by Festo company were selected for our newest study.

THE STUDY

A good background of our test bed and former experimental results of positioning can be found in [9] and [10].

The PAMs were installed horizontally and can be controlled by MPYE-5-M5-010-B type proportional valve made by Festo. Our robust position control method based on sliding-mode control. The linear displacement of the actuator was measured using a LINIMIK MSA 320 type linear incremental encoder with 0,01 mm resolution.

To measure temperature inside and outside the muscle the test-bed was completed two thermocouples type K (Figure 1). Figure 2 shows the block diagram of this positioning system with proportional valve.

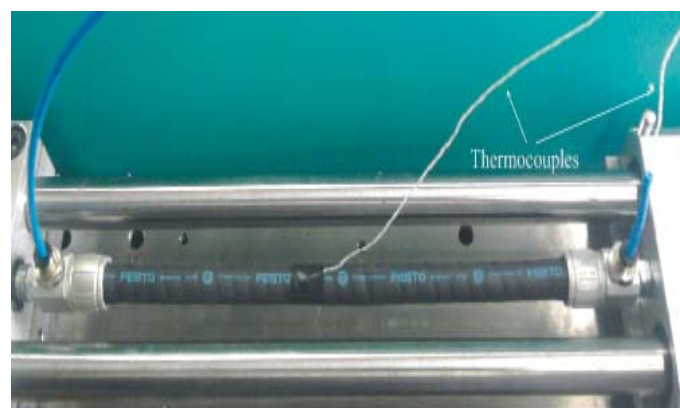


Figure 1. Muscle with two thermocouples

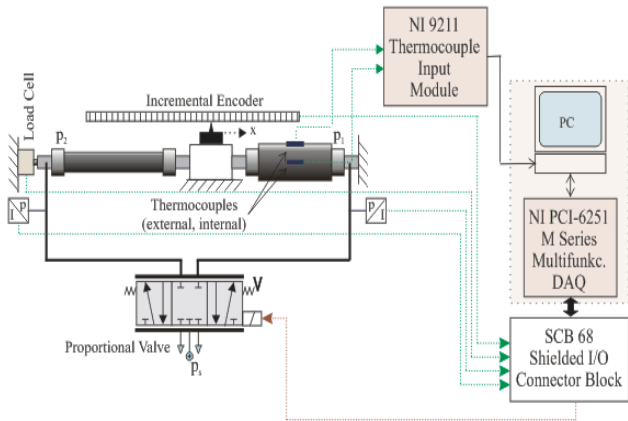


Figure 2. Block diagram of positioning system with proportional valve

The Figure 3 shows data acquisition and positioning that can be achieved in LabVIEW environment. Aside from the desired position the number of samples and the sampling time can also be set. The data can be saved into a text file.

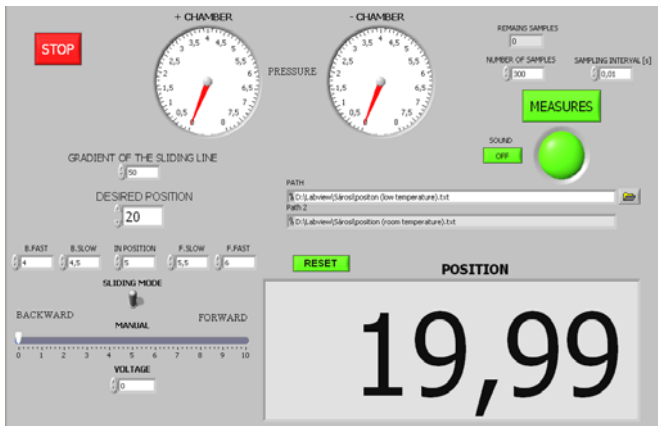


Figure 3 Front panel of LabVIEW program for positioning

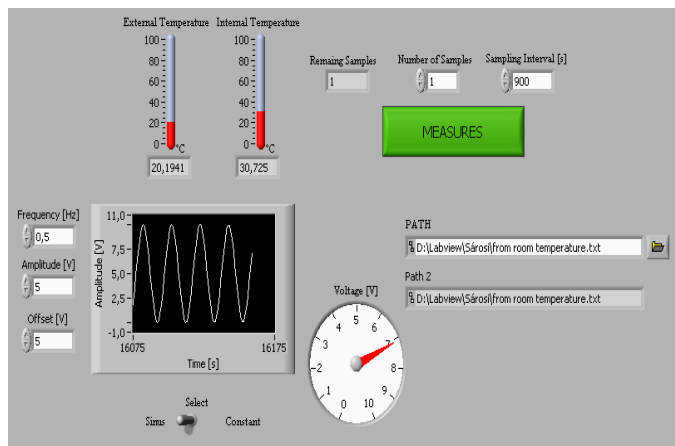


Figure 4. Front panel of LabVIEW program for measuring temperature

The Figure 4 shows the front panel of the LabVIEW program created for temperature measurement. Here the number of samples and sampling time can also be set. During the periodic and automatic working of the muscles the contraction and rate of release can be adjusted with the frequency of the sine wave.

The temperature inside and on the surface of the muscle can be read on the indicators on the screen also it is shown as a number. The measured results are saved in a text file for later processing.

RESULTS AND DISCUSSION

Positioning was first done in room temperature on the pressure of 6 bar. The desired positioning was set to 20 mm, the number of samples was set to 300, while the sampling rate was set to 10 ms, and thus the measurement took 3 s.

Figure 5 shows the positioning as a function of time. It took about 1,85 s for the position to reach the set value. To show the accuracy of positioning the area around the desired position has been magnified (Figure 6). This Figure shows the accuracy of positioning is within 0,01 mm.

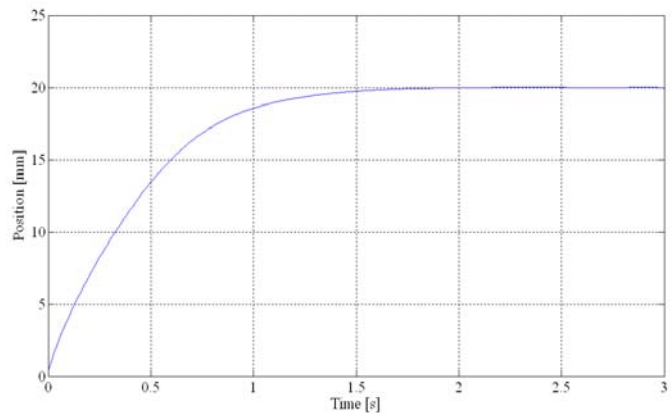


Figure 5. Position as a function of time

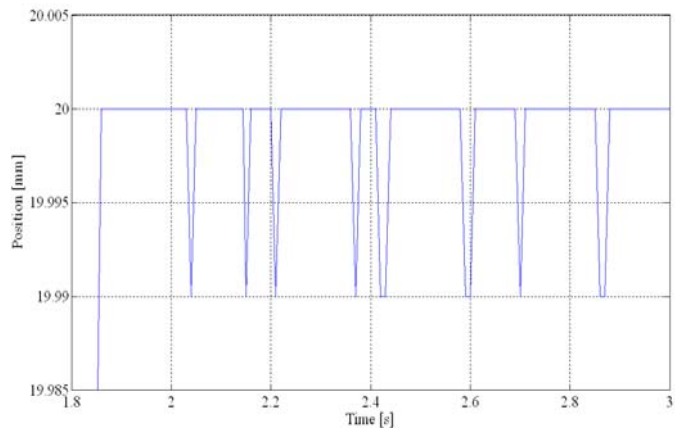


Figure 6. Position as a function of time (enlarged)

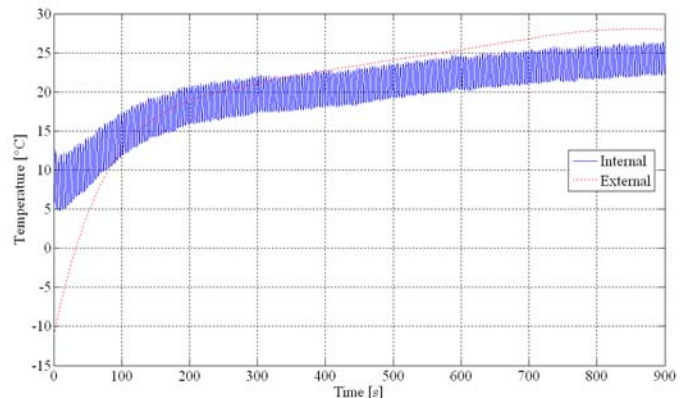


Figure 7. Temperature as a function of time

The periodic working of the muscles was achieved with a 0,5 Hz frequency sine wave. The measurement took 900 s during which the sampling time was 0,25 s, the acquired data is shown in Figure 7. While the surface temperature reached about 28°C, the internal temperature oscillated a lot during contraction and release, for this reason a spline approximation was used for the internal temperature (Figure 8).

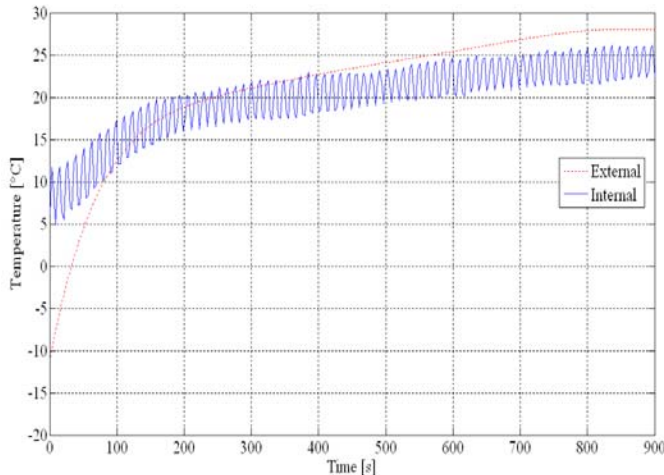


Figure 8. Temperature as a function of time with spline interpolation for internal temperature

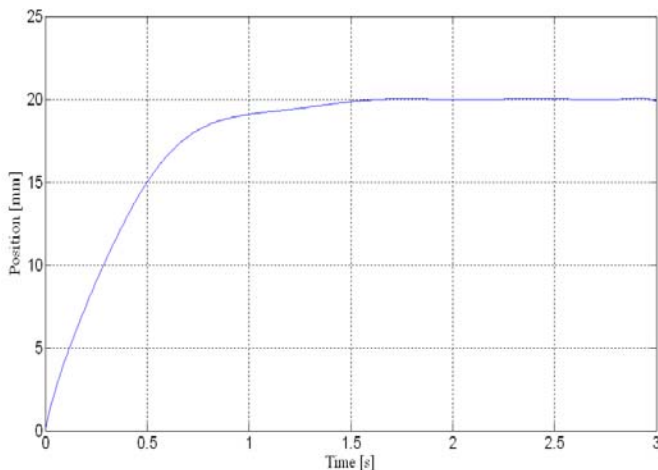


Figure 9. Position as a function of time after work cycle

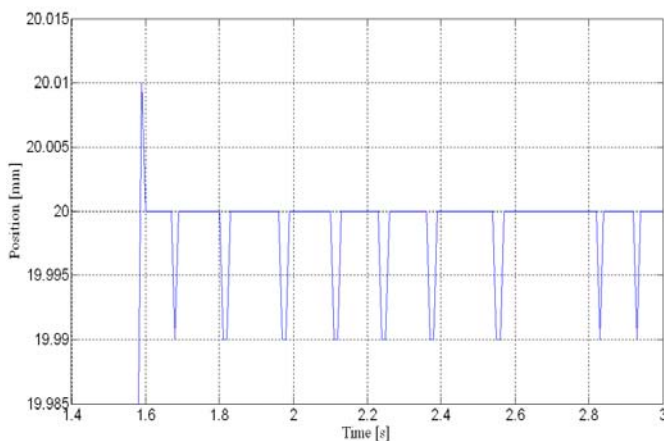


Figure 10. Position as a function of time (enlarged) after work cycle

After a constant temperature was reached positioning was measured on the pressure of 6 bar, too. The result of it is shown in Figure 9. It shows the desired position was reached within 1,6 s. To show the accuracy of positioning the area around the desired position has been magnified (Figure 10.). The accuracy of positioning remained within 0,01 mm.

CONCLUSIONS

From these measurements the conclusion is that the sliding-mode control is rather robust for accurate positioning and the accuracy and time of positioning is more favorable at higher temperature. We plan these investigations will be repeated with different muscles.

REFERENCES

- [1.] Daerden, F. (1999): *Conception and realization of pleated artificial muscles and their use as compliant actuation elements*, PhD Dissertation, Vrije Universiteit Brussel, Faculteit Toegepaste Wetenschappen Vakgroep Werktuigkunde, pp. 5-33.
- [2.] Daerden, F. and Lefeber, D. (2002): *Pneumatic artificial muscles: actuator for robotics and automation*, *European Journal of Mechanical and Environmental Engineering*, Volume 47, pp. 10-21.
- [3.] Caldwell, D. G., Razak, A. and Goodwin, M. J. (1993): *Braided pneumatic muscle actuators*, *Proceedings of the IFAC Conference on Intelligent Autonomous Vehicles*, Southampton, United Kingdom, 18-21 April, 1993, pp. 507-512.
- [4.] Balara, M. and Petík, A. (2004): *The properties of the actuators with pneumatic artificial muscles*, *Journal of Cybernetics and Informatics*, Volume 4, pp. 1-15.
- [5.] Chou, C. P. and Hannaford, B. (1996): *Measurement and modeling of McKibben pneumatic artificial muscles*, *IEEE Transactions on Robotics and Automation*, Volume 12 (1), pp. 90-102.
- [6.] Tondu, B. and Lopez, P. (2000): *Modeling and control of McKibben artificial muscle robot actuator*, *IEEE Control System Magazine*, Volume 20, pp. 15-38.
- [7.] Caldwell, D. G., Medrano-Cerda, G. A. and Goodwin M. (1995): *Control of pneumatic muscle actuators*, *IEEE Control System Magazine*, Volume 15 (1), pp. 40-48.
- [8.] Situm, Z. and Herceg, Z. (2008): *Design and control of a manipulator arm driven by pneumatic muscle actuators*, *16th Mediterranean Conference on Control and Automation*, Ajaccio, France, 25-27 June, 2008, pp. 926-931.
- [9.] Sárosi J., Gyeviki J., Szabó G. and Szendrő P. (2010): *Laboratory Investigations of Fluid Muscles*, *International Journal of Engineering*, *Annals of Faculty of Engineering Hunedoara*, 2010, Volume 8 (1), pp. 137-142.
- [10.] Sárosi J., Gyeviki J., Véha A. and Toman P. (2009): *Accurate Position Control of PAM Actuator in LabVIEW Environment IEEE*, *7th International Symposium on Intelligent Systems and Informatics*, Subotica, Serbia, 25-26 September, 2009, pp. 301-305

AUTHOR & AFFILIATION

József SÁROSI¹

¹ FACULTY OF ENGINEERING, UNIVERSITY OF SZEGED, HUNGARY