

EFFECT OF TEMPERATURE ON POSITIONING OF DIFFERENT PAM ACTUATORS

■ ABSTRACT:

Some researchers have mentioned that temperature creates an important part in the accuracy of positioning of pneumatic artificial muscles (PAMs). However, in literature investigations for measuring temperature inside and outside the PAMs have not been found. This paper presents our robust motion control of these muscle actuators under different temperatures using sliding-mode control.

■ KEYWORDS:

Temperature, pneumatic artificial muscles (PAMs), robust motion control

INTRODUCTION

The working principle of the pneumatic artificial muscles is well described in literature ([1], [2], [3], [4], [5] and [6]).

There are a lot of advantages of these muscles like the high strength, good power-weight ratio, low price, little maintenance needed, great compliance, compactness, inherent safety and usage in rough environments. However, problems with the control of the highly nonlinear pneumatic systems have prevented their widespread use [7]. For this, a fast and robust control necessary to achieve the desired motion. Several control ways have been applied to control different humanoid or robot arms, manipulators, prosthetic and therapy devices driven by pneumatic artificial muscles. The early control methods were based on classical linear controllers and then some modern control strategies have been developed (e. g. adaptive controller, sliding-mode controller, fuzzy controller, neural network controller and others) [8].

The layout of this paper is as follows. Section 2 (The study) is devoted to display our test-bed and the LabVIEW programs. Section 3 (Results and discussion) presents several experimental results. Finally, section 4 (Conclusions) gives the investigations we plan.

Fluid Muscles DMSP-20-200N-RM-RM (with inner diameter of 20 mm and initial length of 200 mm) and DMSP-10-250N-RM-RM (with inner diameter of 10 mm and initial length of 250 mm) produced by Festo company were selected for our newest study.

THE STUDY

A good background of our test bed and former experimental results of positioning can be found in [9] and [10].

The PAMs were installed horizontally and can be controlled by MPYE-5-M5-010-B type proportional valve made by Festo. Our robust position control method based on sliding-mode control. The linear displacement of the actuator was measured using a LINIMIK MSA 320 type linear incremental encoder with 0.01 mm resolution.

To measure temperature inside and outside the muscle the test-bed was completed two thermocouples type K (Figure 1). Figure 2 shows the block diagram of this positioning system with proportional valve.

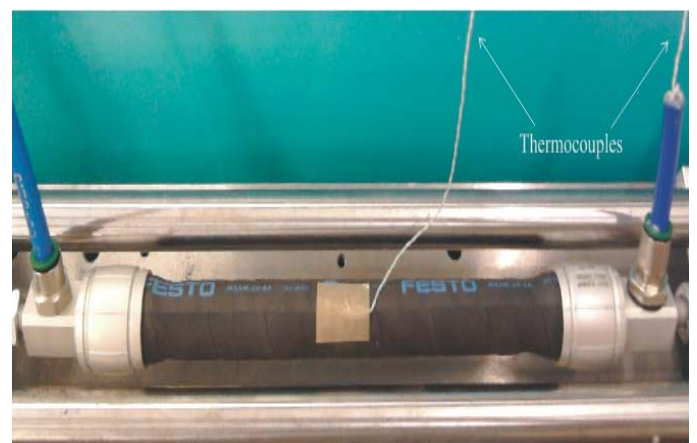


Figure 1 Muscle with two thermocouples

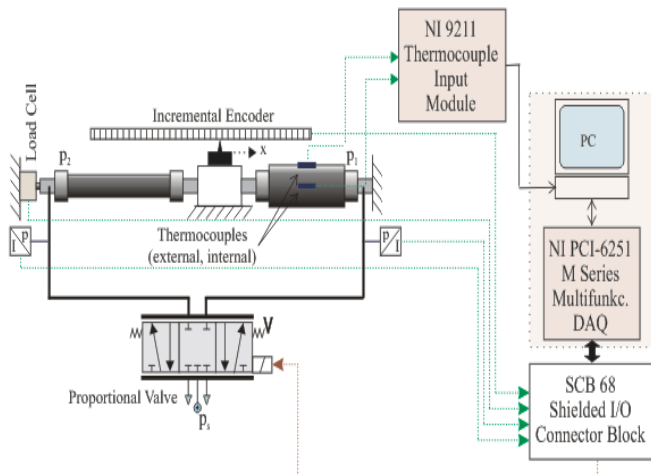


Figure 2 Block diagram of positioning system with proportional valve

The Figure 3 shows data acquisition and positioning that can be achieved in LabVIEW environment. Aside from the desired position the number of samples and the sampling time can also be set. The data can be saved into a text file.

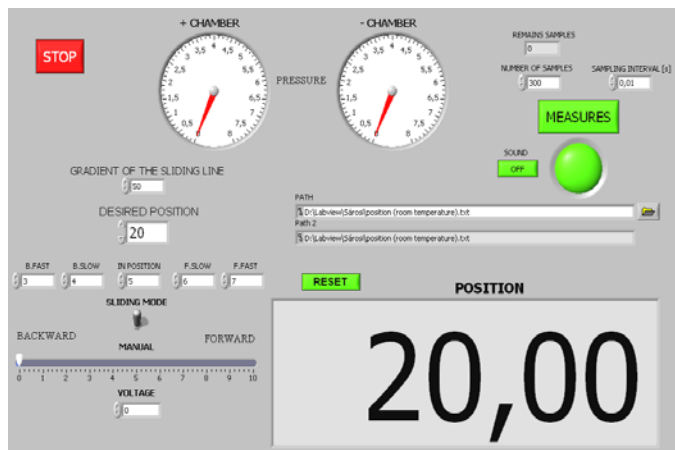


Figure 3 Front panel of LabVIEW program for positioning

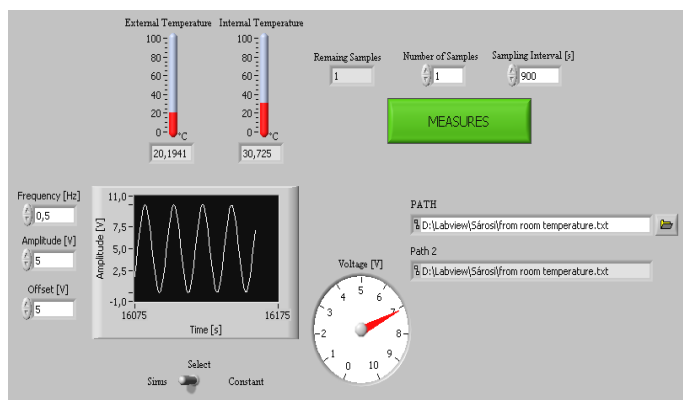


Figure 4 Front panel of LabVIEW program for measuring temperature

The Figure 4 shows the front panel of the LabVIEW program created for temperature measurement. Here the number of samples and sampling time can also be set. During the periodic and automatic working of the

muscles the contraction and rate of release can be adjusted with the frequency of the sine wave. The temperature inside and on the surface of the muscle can be read on the indicators on the screen also it is shown as a number. The measured results are saved in a text file for later processing.

RESULTS AND DISCUSSION

Firstly, the positioning was done with DMSP-20-200N-RM-RM type Fluid Muscle in room temperature on the pressure of 6 bar. The desired positioning was set to 20 mm, the number of samples was set to 300, while the sampling rate was set to 10 ms, thus the measurement took 3 s.

Figure 5 shows the positioning as a function of time. It took about 2 s for the position to reach the set value. To show the accuracy of positioning the area around the desired position has been magnified (Figure 6). This Figure shows the accuracy of positioning is within 0.01 mm.

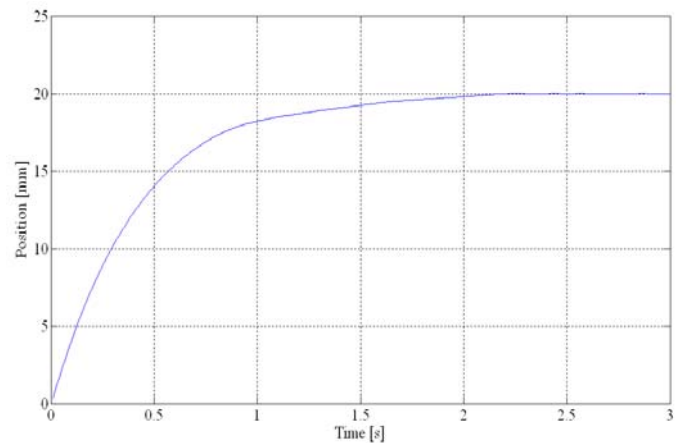


Figure 5 Position as a function of time

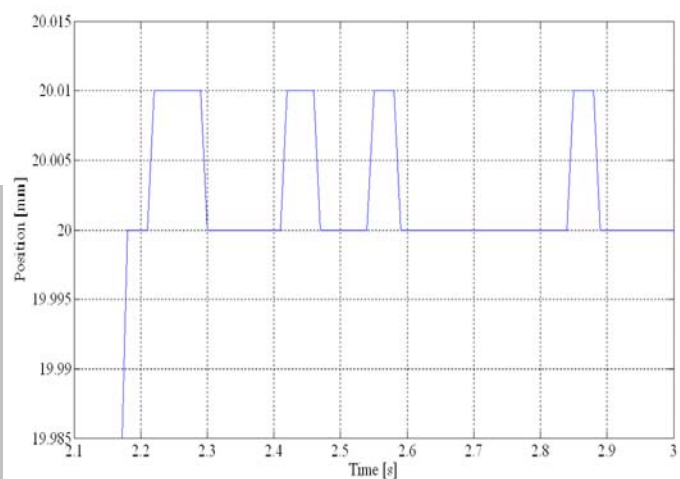


Figure 6 Position as a function of time (enlarged)

The periodic working of the muscles was achieved with a 0.5 Hz frequency sine wave. The measurement took 900 s during which the sampling time was 0.25 s, the acquired data is shown in Figure 7. While the surface temperature reached about 33°C, the internal temperature oscillated a lot during contraction and release, for this reason a spline approximation was used for the internal temperature (Figure 8).

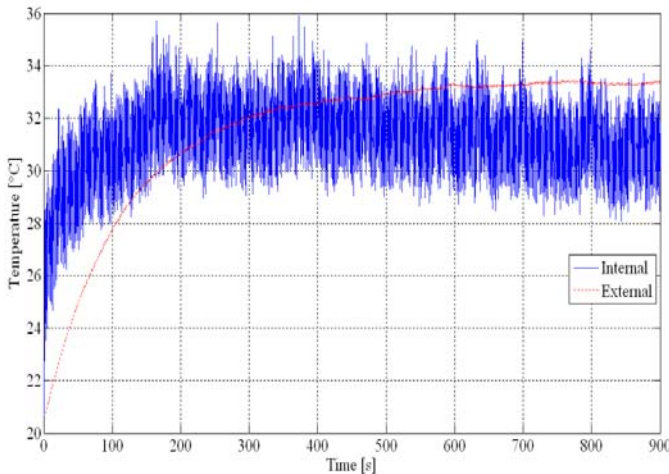


Figure 7 Temperature as a function of time

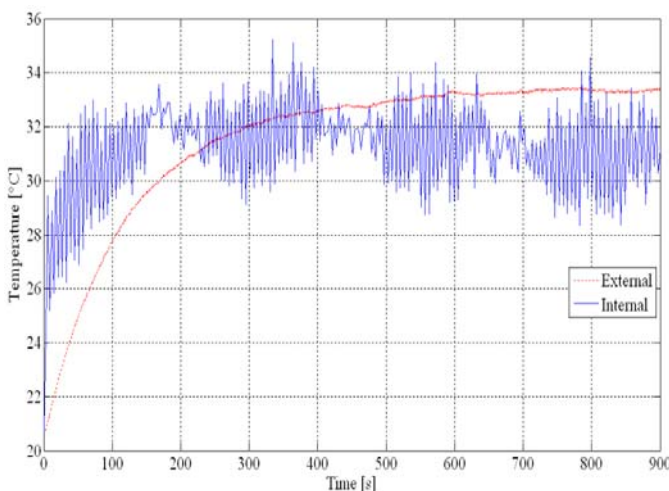


Figure 8 Temperature as a function of time with spline interpolation for internal temperature

After a constant temperature was reached positioning was measured on the pressure of 6 bar, too. The result of it is shown in Figure 9. It shows the desired position was reached within 0.8 s. To show the accuracy of positioning the area around the desired position has been magnified (Figure 10). The accuracy of positioning remained within 0.01 mm.

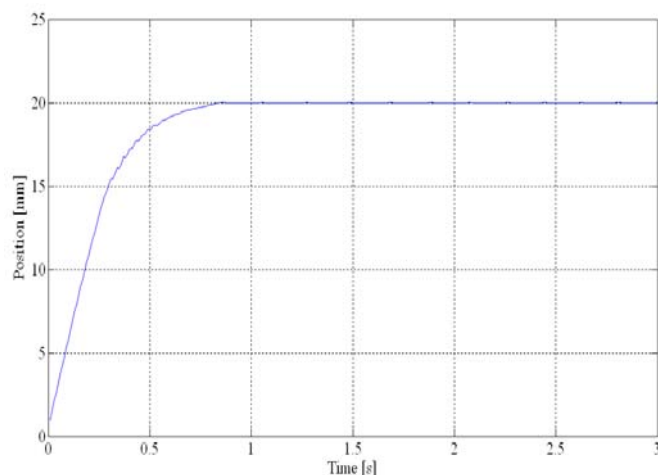


Figure 9 Position as a function of time after work cycle

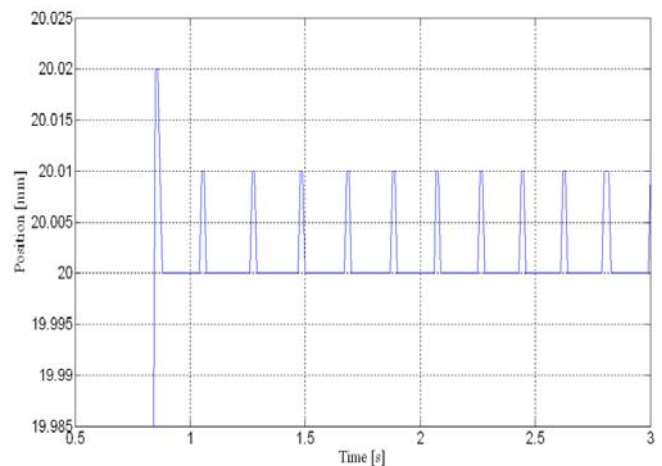


Figure 10 Position as a function of time (enlarged) after work cycle

To compare the previous results the investigations were repeated with DMSP-10-250N-RM-RM type Fluid Muscles. In room temperature the desired positioning was set to 10 mm, the number of samples was set to 300, while the sampling rate was set to 10 ms, thus the measurement took 3 s. Figure 11 and Figure 12 shows the experimental results. It took about 1.05 s for the position to reach the set value and the accuracy of positioning is within 0.01 mm.

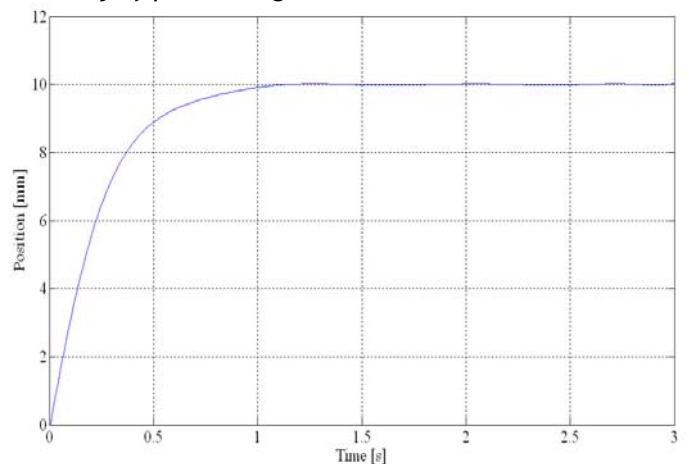


Figure 11 Position as a function of time

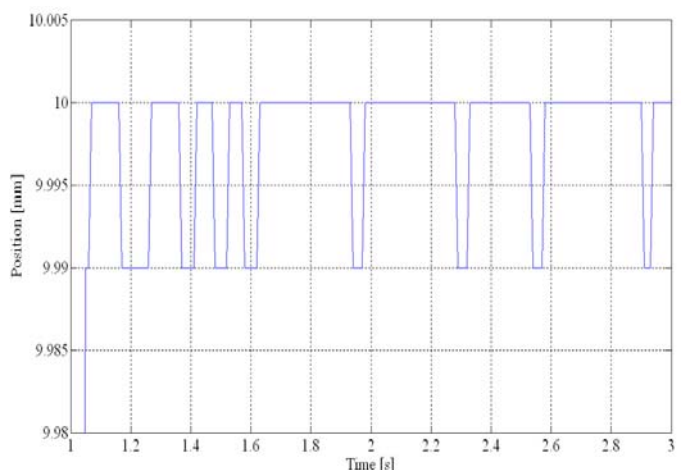


Figure 12 Position as a function of time (enlarged)

The periodic working of the muscles was achieved with a 0.5 Hz frequency sine wave. The measurement took 900 s during which the sampling time was 0.25 s, the acquired data is shown in Figure 13 and Figure 14. While the surface temperature reached about 31 °C, the internal temperature oscillated a lot during contraction and release, for this reason a spline approximation was used for the internal temperature.

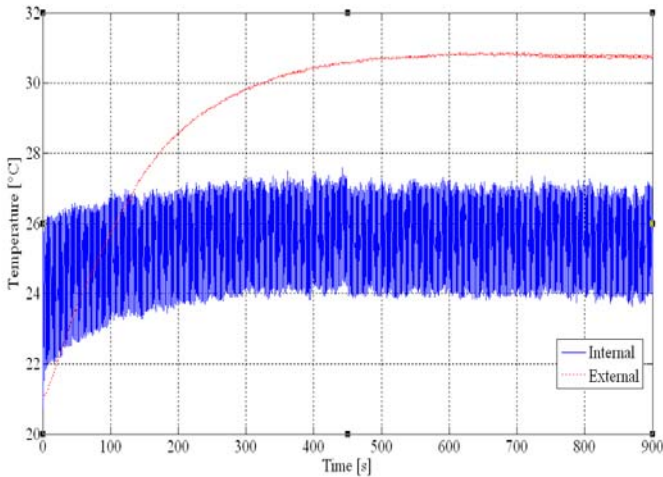


Figure 13 Temperature as a function of time

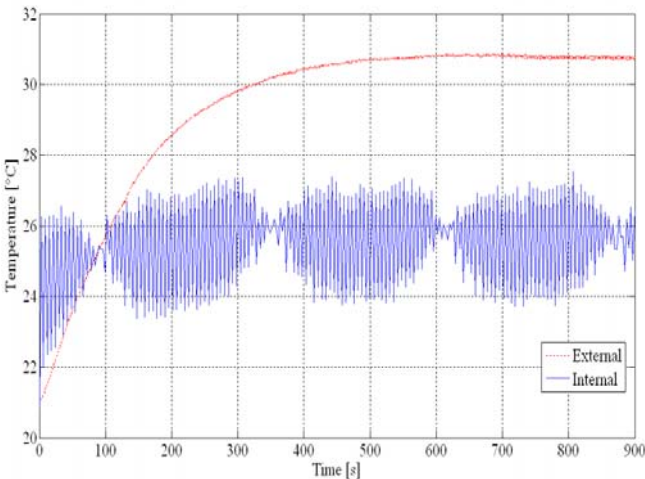


Figure 14 Temperature as a function of time with spline interpolation for internal temperature

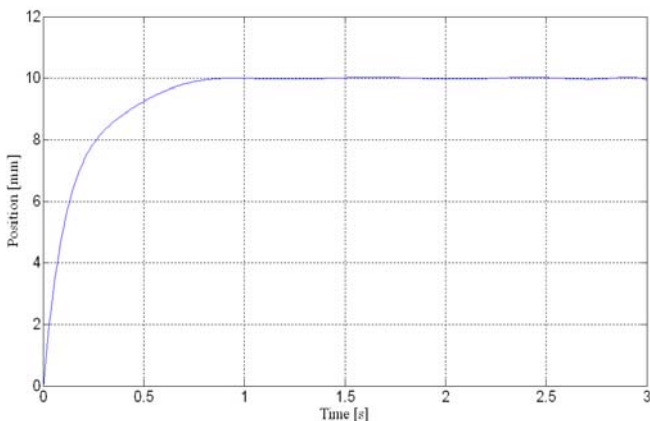


Figure 15 Position as a function of time after work cycle

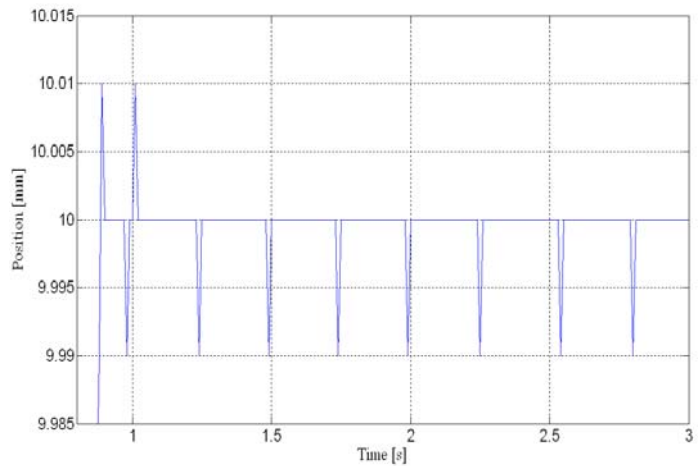


Figure 16 Position as a function of time (enlarged) after work cycle

After a constant temperature was reached positioning was repeated. The results of it are shown in Figure 15 and Figure 16. The desired position was reached within 0.9 s. and the accuracy of positioning remained within 0.01 mm.

CONCLUSIONS

From these measurements the conclusion is that the ideal working temperature of the muscles is not room temperature, but greater than that. The accuracy and time of positioning is more favorable at higher temperature and independent from the geometric properties. We plan these investigations will be repeated with a third Fluid Muscle (DMSP-20-400N-RM-RM type Fluid, with inner diameter of 20 mm and initial length of 400 mm).

REFERENCES

- [1.] Daerden, F. (1999): Conception and realization of pleated artificial muscles and their use as compliant actuation elements, PhD Dissertation, Vrije Universiteit Brussel, Faculteit Toegepaste Wetenschappen Vakgroep Werktuigkunde, pp. 5-33.
- [2.] Daerden, F. and Lefeber, D. (2002): Pneumatic artificial muscles: actuator for robotics and automation, *European Journal of Mechanical and Environmental Engineering*, Volume 47, pp. 10-21.
- [3.] Caldwell, D. G., Razak, A. and Goodwin, M. J. (1993): Braided pneumatic muscle actuators, *Proceedings of the IFAC Conference on Intelligent Autonomous Vehicles*, Southampton, United Kingdom, 18-21 April, 1993, pp. 507-512.
- [4.] Balara, M. and Petik, A. (2004): The properties of the actuators with pneumatic artificial muscles, *Journal of Cybernetics and Informatics*, Volume 4, pp. 1-15.
- [5.] Chou, C. P. and Hannaford, B. (1996): Measurement and modeling of McKibben pneumatic artificial muscles, *IEEE Transactions on Robotics and Automation*, Volume 12 (1), pp. 90-102.



- [6.] Tondou, B. and Lopez, P. (2000): Modeling and control of McKibben artificial muscle robot actuator, *IEEE Control System Magazine*, Volume 20, pp. 15-38.
- [7.] Caldwell, D. G., Medrano-Cerda, G. A. and Goodwin M. (1995): Control of pneumatic muscle actuators, *IEEE Control System Magazine*, Volume 15 (1), pp. 40-48.
- [8.] Situm, Z. and Herceg, Z. (2008): Design and control of a manipulator arm driven by pneumatic muscle actuators, 16th Mediterranean Conference on Control and Automation, Ajaccio, France, 25-27 June, 2008, pp. 926-931.
- [9.] Sárosi J., Gyeviki J., Szabó G. and Szendrő P. (2010): Laboratory Investigations of Fluid Muscles
- [10.] *International Journal of Engineering, Annals of Faculty of Engineering Hunedoara*, 2010, Volume 8 (1), pp. 137-142.
- [11.] Sárosi J., Gyeviki J., Véha A. and Toman P. (2009): Accurate Position Control of PAM Actuator in LabVIEW Environment
- [12.] IEEE, 7th International Symposium on Intelligent Systems and Informatics, Subotica, Serbia, 25-26 September, 2009, pp. 301-305

AUTHORS & AFFILIATION

¹József SÁROSI,
²Sándor CSIKÓS

¹FACULTY OF ENGINEERING, UNIVERSITY OF SZEGED
²FACULTY OF SCIENCE AND INFORMATICS, UNIVERSITY OF SZEGED,
HUNGARY



ACTA TECHNICA CORVINIENSIS
- BULLETIN of ENGINEERING
ISSN: 2067-3809 [CD-Rom, online]
copyright © University Politehnica Timisoara,
Faculty of Engineering Hunedoara,
5, Revolutiei,
331128, Hunedoara,
ROMANIA
<http://acta.fih.upt.ro>